

rad-sure™ UVA 3J

UVA illumination indicators

Rad-Sure and Pathogen Reduction

As your blood components filter to storage bags, Rad-Sure UVA 3J can now move with it

Features of Rad-Sure UVA 3J indicators



- Easy to use and interpret
- Contains UVA-sensitive film
- ISBT bar-coded lot numbers

Benefits of Rad-Sure UVA 3J indicators

- Reduces operator errors
- Provides positive, visual verification of illumination
- Ensures patient safety




Examples of Rad-Sure UVA 3J indicators before and after illumination

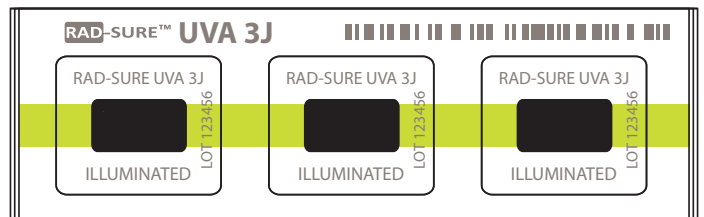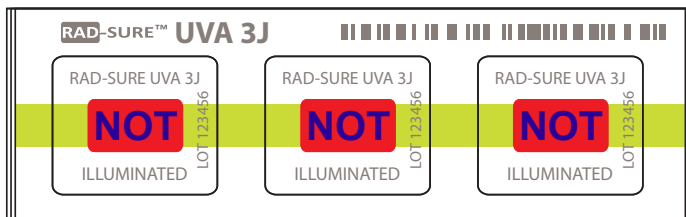

Ordering information for UVA indicators

Version	Product Code	Packaging
Rad-Sure UVA 3J indicators ¹	892206	200 / Box

¹ To be used only in the INTERCEPT™ UVA illuminator. INTERCEPT™ is a registered trademark of Cerus.

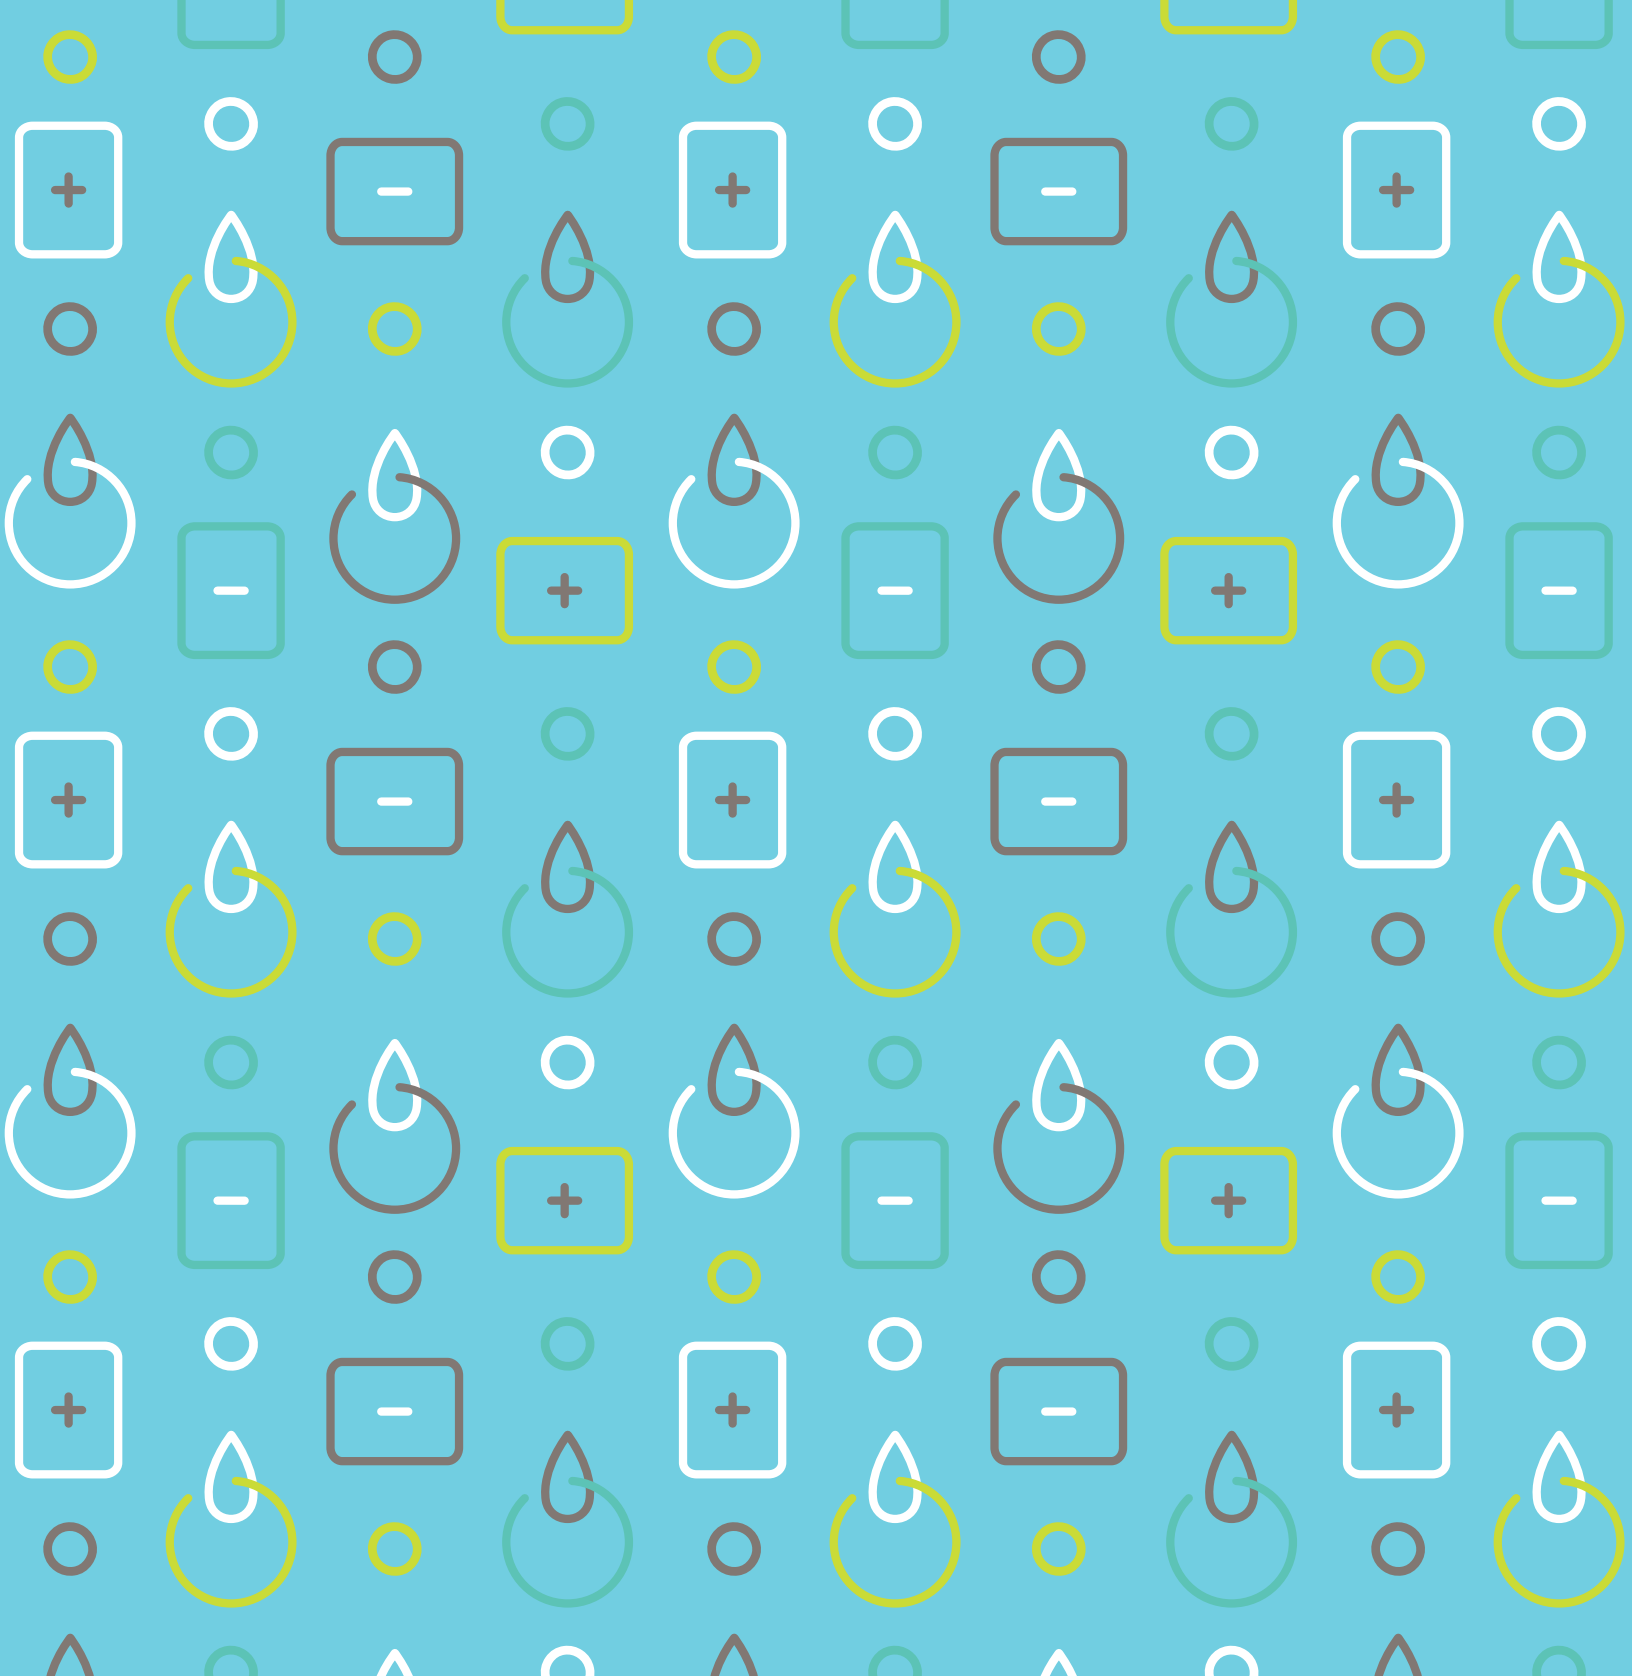

Domestic Orders and Inquiries
AdvancedOrders@ashland.com

International Orders and Inquiries
AdvancedMaterialsOrders@ashland.com

ashland.com/contact

® Registered trademark, Ashland or its subsidiaries, registered in various countries
™ Trademark, Ashland or its subsidiaries, registered in various countries
© 2017, Ashland / PHA17-1012

The information contained in this brochure and the various products described are intended for use only by persons having technical skill and at their own discretion and risk after they have performed necessary technical investigations, tests and evaluations of the products and their uses. Certain end uses of these products may be regulated pursuant to rules or regulations governing medical devices, drug uses, or pesticidal or antimicrobial uses. It is the end user's responsibility to determine the applicability of such regulations to its products.

All statements, information, and data presented herein are believed to be accurate and reliable, but are not to be taken as a guarantee of fitness for a particular purpose, or representation, express or implied, for which seller assumes legal responsibility. No freedom to use any patent owned by Ashland, its subsidiaries, or its suppliers is to be inferred.

